


The following pictures are for reference only.

### Front view

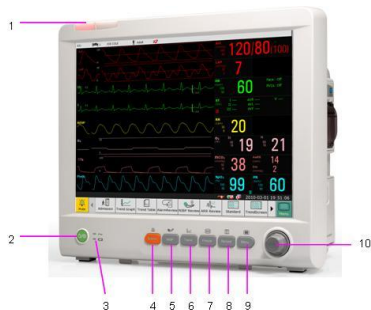


- 1 Alarm Indicator
- 2 Power Supply Switch
- 3 Battery Indicator
- 4 Mute
- 5 Start / Stop NIBP Measurement
- 6 Trend
- 7 Freeze / Unfreeze
- 8 Start / Stop Recording
- 9 Menu

### Side view



- 10 Trim Knob
- 11 Sensor Port
- 12 AG Fixation Bracket
- 13 Recorder Door
- 14 Battery Door

### Back view

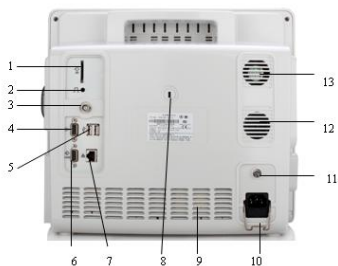

- 1 SD Card
- 2 Nurse Call
- 3 Defibrillator synchronization / Analog Output
- 4 VGA Output
- 5 USB Interface
- 6 RS232 Interface
- 7 Network Interface
- 8 Anti-theft Lock
- 9 Heat Emission Hole
- 10 Security Lock
- 11 Grounding Equipotential Terminal
- 12 Speaker
- 13 Fan

The following functions can be performed by clicking on the hot keys on the screen. When selecting these items, for the touch screen, the user can touch the screen directly to perform the function; for non-touch screen, the user can turn the trim knob to perform the function. Of course, the user can perform all the functions by using the main menu key.

# 1 On-Screen Keys and Their Functions

## Permanent Keys



Display the main setup menu



To reset the alarm.

## Shortcut Keys



Admit a patient



Review trend graph



Review trend table



Review the alarm event



Access the NIBP review



Access ARR review



Enter the standard screen



Enter the trend screen



Enter the OxyCRG screen



Enter the large font screen



Set the module switch



Change the key volume



Adjust screen brightness



Zero the IBP sensor



Alarm setup



Change the beat volume



Enter standby mode



Enter night mode



Switch to the vital screen



Select it by the knob to enable the touch screen operation

## 2 Basic Operation

Attach the ECG cable to the connector, perform skin preparation and attach the leads to the patient. Attach the SpO<sub>2</sub> cable to the connector and the sensor to the patient. Attach one end of the NIBP tube to the connector; select a cuff with a suitable size and apply to the patient; then connect the other end of the tube to the cuff. Press the On/Off button to turn on the monitor. For more information, please refer to the user manual.

## 3 Considerations

1. Before NIBP measurement, please check whether patient type in information area is correct. Wrong type may cause inaccurate measurement results or serious injuries. For this reason, please access **Menu > Patient Setup > Patient Info > Type** to select the correct patient type. For automatic NIBP measurement, please first access **NIBP Setup** to select **Interval** to set the interval between measurements.
2. If the ECG waveforms appear intermittently or there is obvious interference on the ECG signals, it is usually because the patient skin has not been well cleaned or the ECG electrodes are defective. In this situation, please carefully clean the skin and select effective electrodes.
3. The device must be connected to the ground to avoid the interference signal.
4. Be careful when inserting paper. Avoid damaging the thermo-sensitive print head. Do not leave the recorder door open unless inserting paper or troubleshooting.
5. Recharge the batteries at a minimum of every 6 months when they are stored.